


# ***Integrated Veterinary System***

## ***Operator's Manual***

***P/N #02026 Rev B***

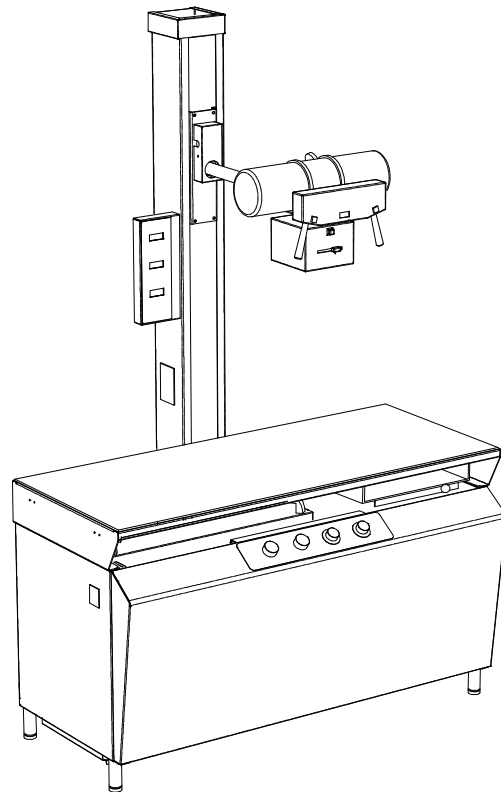

**SUMMIT INDUSTRIES INC.  
2901 W. Lawrence Avenue  
Chicago, IL 60625  
1-800-972-9776**



TABLE OF CONTENTS

**1.0 INTRODUCTION..... 1**

**2.0 PRECAUTIONS ..... 2**

    2.1 Installation ..... 2

    2.2 Operation..... 2

**3.0 GENERAL PRODUCT OVERVIEW..... 4**

    3.1 Major Components ..... 4

    3.2 Specifications ..... 6

    3.3 Options ..... 8

**4.0 FUNCTIONS ..... 9**

    4.1 Getting Started ..... 9

    4.2 Positioning the Tube ..... 9

    4.3 Collimator Operation..... 10

    4.4 Setting Techniques ..... 11

    4.5 Making Exposures ..... 12

    4.6 Prep/Expose Tubestand Status Messages..... 13

**5.0 TECHNICAL DATA ..... 14**

    5.1 Radiation Leakage (Meets Federal Government Standards) ..... 14

    5.2 Rated line voltage: 240 VAC, 60 Hz., single phase. .... 14

    5.3 Range of line voltage regulation at max line current: 1% to 5%. .... 14

    5.4 Maximum line current (based on input voltage of 240 VAC): 140 AMP ..... 14

    5.5 Technique factors that constitute the max. line current: 300 mA @ 125 kVp. .... 14

    5.6 Maximum Deviation of technique factors:..... 14

**6.0 CLEANING THE *Integrated Veterinary System*..... 15**

**7.0 SCHEDULED DEALER MAINTENANCE..... 16**

    7.1 X-Ray Generator Maintenance ..... 16

    7.2 X-Ray Tube Housing ..... 16

    7.3 Collimator ..... 16

    7.4 Tubestand ..... 17

    7.5 Other ..... 17



<b>8.0 TROUBLESHOOTING.....</b>	<b>18</b>
8.1 Error Message .....	18
8.2 No Exposure.....	18
8.3 Collimator light bulb burned out.....	18
8.4 No digital display .....	20
8.5 Circuit tripping.....	20
8.6 Full kVp range inaccessible.....	20
8.7 Poor film quality .....	20
<b>9.0 WARRANTY NOTICE.....</b>	<b>21</b>





## 1.0 INTRODUCTION

Congratulations! You've purchased an ***Integrated Veterinary System*** Veterinary X-Ray System. Summit Industries' product line has long represented a new concept in veterinary radiography by designing the first system to incorporate the x-ray generator into the table. This major innovation led to other significant design breakthroughs yielding the most practical, efficient and compact unit ever created. The result of this innovation and improvement is the ***Integrated Veterinary System*** you have purchased.

Because the ***Integrated Veterinary System*** is so unique, its features and functions are a bit different from those of traditional x-ray systems. The purpose of this manual is to familiarize you with the ***Integrated Veterinary System*** and assist you with operating and maintaining your new system. The manual is divided into indexed sections for quick and easy access to information.

Should a situation arise which cannot be resolved through the troubleshooting procedures described in this manual, please contact the Summit dealer where you purchased your machine for assistance, or call Summit directly at 1-800-972-9776.



## 2.0 PRECAUTIONS

### 2.1 Installation

The ***Integrated Veterinary System*** must be installed and serviced by an authorized Summit dealer. All warranties will be void if such installation or service is performed by persons not authorized by Summit.

### 2.2 Operation

#### 2.2.1 Radiation

X-rays are dangerous to both operator and others in the vicinity unless established safe exposure procedures are strictly observed.

The useful and scattered beams can produce serious, genetic or potentially fatal bodily injuries to any persons in the surrounding area if used by an unskilled operator. Adequate precautions must always be taken to avoid exposure to the useful beam, as well as to leakage radiation from within the source housing or to scattered radiation resulting from the passage of radiation through matter.

Those authorized to operate, test participate in or supervise the operation of the equipment must be thoroughly familiar and comply completely with the currently established safe exposure factors and procedures described in publications such as Sub-Chapter J of Title 21 of the Code of Federal Regulations "Diagnostic X-Ray Systems and their Major Components" and the National Council on Radiation Protection (NCRP) No.33, "Medical X-Ray and Gamma-Ray protection for energies up to 10 MeV-Equipment Design and Use", as revised or replaced in the future.

Failure to observe these warnings may cause serious, genetic or potentially fatal bodily injuries to the operator or those in the area.

#### 2.2.2 Electrical

Only properly trained and qualified personnel should be permitted access to any internal parts. Live electrical terminals may be deadly. Be sure line disconnect switches are opened and other appropriate precautions are taken before opening access doors, removing enclosure panels, or attaching accessories.



Do not remove the flexible high tension cables from the x-ray tube housing or high tension generator or the access covers from the generator until the main and auxiliary power supplies have been disconnected.

When disconnecting high-voltage cables, they must be grounded immediately in order to dissipate any electrical charge that may remain on the cables or the tube.

Failure to comply with the foregoing may result in serious or potentially fatal bodily injuries to the operator or those in the area.

### 2.2.3 Mechanical


All of the movable assemblies and parts of x-ray equipment should be operated with care. Only properly trained and qualified personnel should be permitted access to any internal parts.

Particular care should be taken when servicing the inside of the tubestand. There is an extreme threat of mechanical pinching between the vertical slide and counterweight due to their close proximity and opposite directions of motion.



### 3.0 GENERAL PRODUCT OVERVIEW

#### 3.1 Major Components

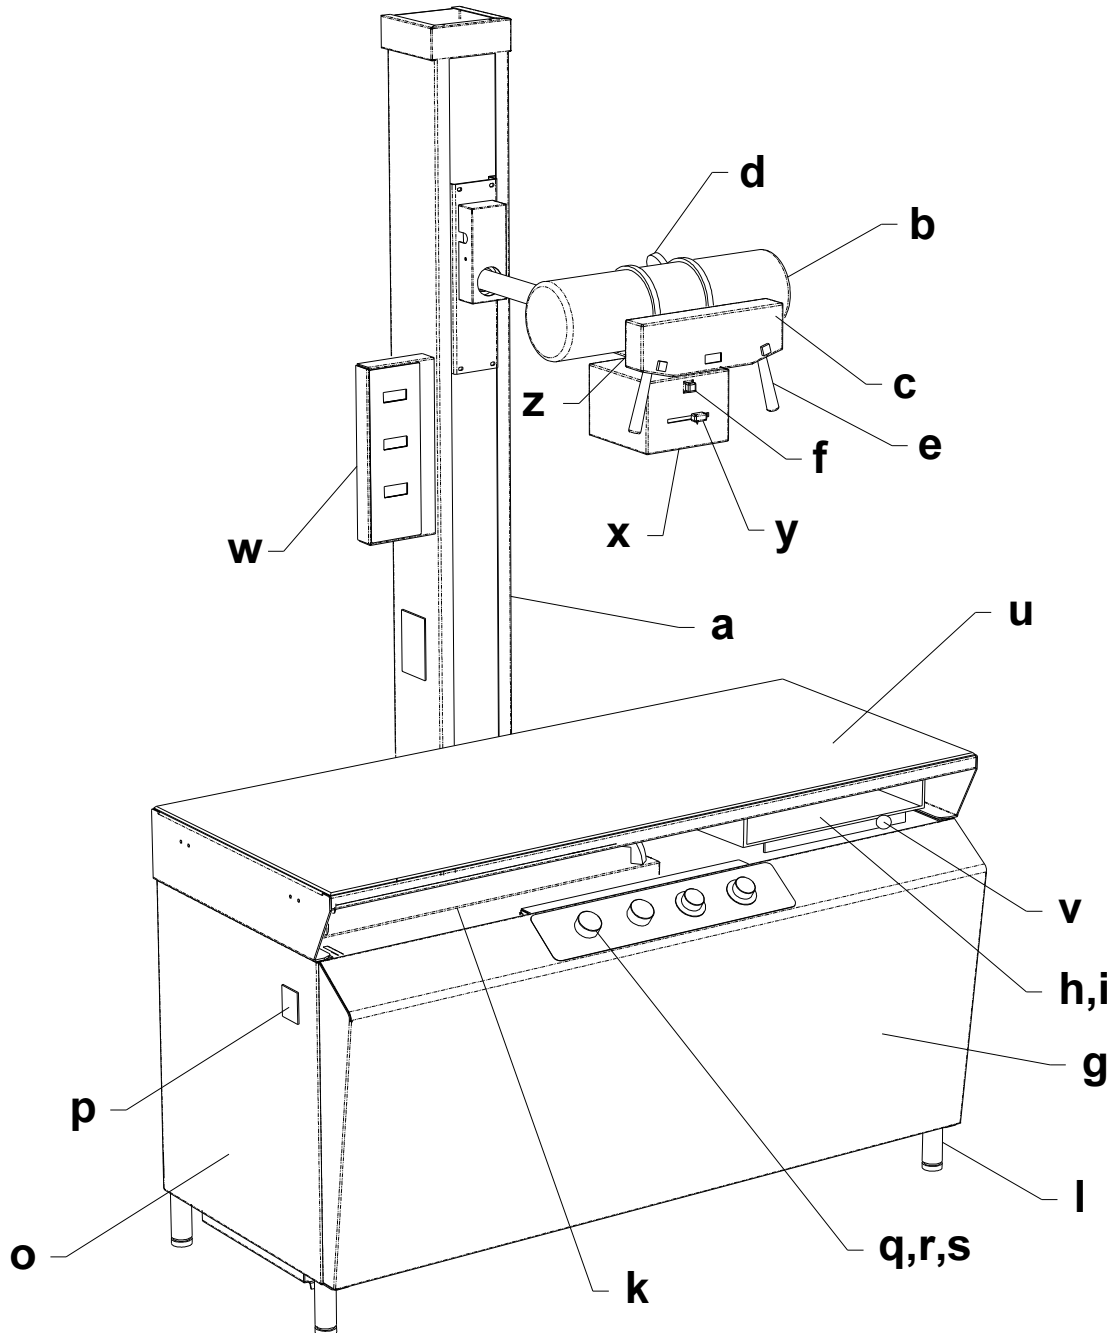



- a. Tubestand - Supports collimator and x-ray tube. Moves both horizontally and vertically with mechanical locks.
- b. X-Ray Tube
- c. Angulation Dial - Displays degree of x-ray tube angulation.
- d. Angulation Lock - When knob is loosened allows angulation of x-ray tube.
- e. Handle Bars - Used to move tube vertically or to angle the tube.
- f. Light Switch Button - Turns collimator bulb on and off.
- g. Removable Front Cover.
- h. Grid Cabinet - Lead-lined cabinet holds cassette tray and grid.
- i. Grid, mounted to upper carriage of grid cabinet, absorbs scatter radiation for improved film clarity.
- k. X-Ray Generator.
- l. Leveling Feet
- o. Table Base - All steel, welded construction.
- p. ON/OFF circuit breaker
- q. kVp Dials - One for major adjustment (15 kVp increments); One for minor (2 kVp increments).
- r. mA Dial - Adjusts mA. Two stations; 100 when using small focal spot and 300 when using large focal spot of the x-ray tube.
- s. Time Dial - Adjusts time. 18 stations available: 1/120, 1/60, 1/40, 1/30, 1/24, 1/20, 1/15, 1/12, 1/10, 1/8, 3/20, 1/5, 1/4, 2/5, 1/2, 5/8, 3/4, 1
- u. Table Top - 24" x 56" of Formica
- v. Tubestand/Grid Cabinet Interlock - When engaged, allows tubestand, grid cabinet and cassette tray to move together.
- w. Display box – Indicator of kVp, mAs and generator status.
- x. Collimator - Controls size and rectangular shape of primary beam emitted from x-ray tube and provides coincident light field.



- y. Collimator Shutter Adjustment knobs for controlling size of x-ray field.
- z. Swivel Mounting Plate - Allows collimator to be rotated.

## 3.2 Specifications

### 3.2.1 INTEGRATED GENERATOR

- Table-front access to control.
- 300 mA at 125 kVp.
- Dual-digital timer with 18 time stations (1/120 to 1 second).
- Adjustable solid state audio exposure signal.
- SCR contactor.
- Programmable tube protect system.
- Tube overload sensor.
- Independent kVp and mA adjustment circuits for each mA station.
- Two mA stations: 100S and 300L
- mA overload protection.
- 64 kVp stations (40 to 125).
- kVp selection, major 15 kVp increments, minor 2 kVp increments.
- mA, time and kVp knobs.
- Built-in kVp compensation.
- Easy-access exposure count display
- Filament stabilization.
- 16-foot line cable; 4-foot control-to-transformer cable.
- Integral 24-Volt A.C. power supply.
- Programmable line frequency 50 or 60 Hz.
- Programmable power saving mode.



### 3.2.2 TABLE / TUBESTAND

- Enclosed, integrated table. Removable 24" x 53" top.
- Welded base construction.
- Full-travel, lead-lined grid cabinet.
- 103-line, 8:1 aluminum grid.
- Grid cabinet/tubestand interlock.
- Tubestand-mounted digital kVp, mAs and status displays.
- Attached, counterbalanced tubestand; travels full table length.
- Angulation dial and operator handles.
- Two position foot switch.

### 3.2.3 CASSETTE HOLDER

- Easy-fit, removable, ABS plastic holder.
- Accepts 8" x 10", 10" x 12" and 14" x 17" cassettes in either direction.

### 3.2.4 TUBE

- 1.0-2.0 mm focal spots; 140,000 H.U.

### 3.2.5 CABLES

- 10' Max-Flex high voltage cables. Federal terminations.

### 3.2.6 COLLIMATOR

- Manual with light field.
- Swivel-mount.
- 90-second bulb "on" time.
- Gradual turn off warning (Soft Start Bulb Life feature).



### 3.3 Options

#### 3.3.1 TABLE OPTIONS

- Exposure foot switch.
- 12" table-top extension. Specify right or left (fixed top only).
- Upgrade grid to 10:1, 103 line.
- Animal restraining device.

#### 3.3.2 TUBE / COLLIMATOR OPTIONS

- 0.6-1.5 mm; 200,000 H.U.
- Programmable lamp times - 30, 60, 90, and 120 seconds.

#### 3.3.3 OTHER OPTIONS

- Remote exposure hand switch.
- Standard manual tray with sliding jaws; accepts all cassette sizes up to 14" x 17".



## 4.0 FUNCTIONS

### 4.1 Getting Started

1. Power Switch - To turn the generator on, move the circuit breaker switch to the up position. The switch is located at the left side of the table base.

It is a good idea to turn the unit off at the end of each day. This ultimately will extend your system's life. If power saving mode is selected, the unit turns off automatically.

2. Generator Warm up - When the generator is first turned on after being turned off for two hours or more, the tubestand display will indicate "COLD". After ten minutes this display will change to "READY" which will scroll across the tubestand status window. The generator will take exposures when "COLD", but the outputs will be most accurate when the display indicates "READY". For consistent films wait for the "READY" indicator prior to taking exposures.
3. Tube Warm up - It is recommended that you warm up the unit prior to the first higher-powered exposure to prolong tube life. This is done by taking a series of three, 1/10 second exposures using the 300 mA station. Start with a kVp of 70 and increase to 80; then 90. Exposures should be spaced at least 20 seconds apart.
4. Loading Cassettes - Three sizes of cassettes can be used: 8" x 10", 10" x 12" and 14" x 17". Simply place the cassette into the specially-formed grooves of the tray. It will accept the cassette in either lengthwise or crosswise position.

### 4.2 Positioning the Tube

1. Moving the Grid Cabinet - The grid cabinet will move in tandem with the tubestand, assuring alignment of the primary beam to the center of the film. The grid cabinet can be positioned anywhere along the entire length of the table. Grasp the tubestand handle bars, release the longitudinal lock and move to the desired location.
2. Disengaging the Grid Cabinet - Alternatively, the grid cabinet may be moved independent of the tubestand. Release the interlock by pulling out the spring-loaded lever extending from the grid cabinet. The grid cabinet may then move while the tubestand remains stationary. To re-engage the interlock, position grid cabinet in-line



with tubestand. The interlock is engaged when you hear a metallic "click" sound and feel the interlock mechanism move into place.

3. Vertical Movement - The tube can be moved to a variety of heights above the table top. For convenience, SID markers indicate 40" positions from the table top or the grid cabinet.
4. Angulation - Release the lock, which is located on the right side of the tube arm. Grasp the handle bars and turn the tube to proper angle. Turn the lock handle clockwise to hold tube position. The degree of rotation is indicated by the dial located between the handle bars.

#### 4.3 Collimator Operation

1. Light Field - Once the tube is positioned relative to the grid cabinet, press the light button on the front of the collimator. A light field will appear. The position of the light field prior to exposure indicates the position of x-ray field during exposure. **WARNING! DO NOT LOOK DIRECTLY INTO LIGHT SOURCE AS RETINA DAMAGE COULD RESULT.**
2. Programmable Lamp Times - Lamp gradually turns off in one of the following selectable times: 30, 60, 90, 120 seconds. The factory setting is 90 seconds. If you push the button during the lamp's power down ramp, a new "on" cycle starts.
3. Collimator Adjustment - Use the sliding knobs to move the shutters. Scales indicate knob positions that correspond to common cassette sizes. Use the pointer to quickly move shutters into relative position, then fine tune to collimate the x-ray beam to the area of radiographic interest.
4. Swivel Movement - When doing table top work, you may want to swivel the collimator to avoid awkward patient positioning. Simply swivel the collimator to the preferred position.

**WARNING:** Do not touch the black lamp cover at the rear of the collimator as it gets quite hot. The collimator hesitates at the 0° and 90° positions for correct re-alignment. This is in order to help find these position accurately.



#### 4.4 Setting Techniques

1. mA - Adjust mA by moving the pointer to either 100S or 300L

When set at 100 mA, the small tube focal spot (1.0 mm in standard tube) is used, yielding a more finely detailed image. At 300 mA, the large focal spot (2.0 mm in standard tube) is used.

2. kVp - Two knobs control kVp - one for coarse adjustments of 15 kVp increments and one for fine tuning with 2 kVp adjustments.

Turn the knobs to select the desired kVp.

The kVp value is displayed on the tubestand-mounted display.

3. Time - The time dial can be set at any of 18 stations; these are marked both in fractions of seconds and in natural numbers: 1/120, 1/60, 1/40, 1/30, 1/24, 1/20, 1/15, 1/12, 1/10, 1/8, 3/20, 1/5, 1/4, 2/5, 1/2, 5/8, 3/4, 1 seconds.



#### 4.5 Making an X-Ray Exposure.

**Note:** If it is desired, to view the total number of X-ray exposures, simply turn the KVP major, KVP minor & mA selector knobs fully counter-clockwise, the bottom display will indicate "EXPO". The KVP display and the mAs display will indicate the total number of exposures taken on this x-ray control.

##### 1. Making Exposures with the Standard Foot Switch

There are two ways to make a x-ray exposure with the 2-position footswitch.

###### Prep and Expose

When proper patient position is achieved, partially depress the footswitch to the first position and hold, activating the x-ray tube prep cycle. When "PREP" is displayed on the Tubestand, watch the patient for respiration phase or proper restraint. At the desired moment, make the x-ray exposure by fully depressing the footswitch to the second position. An audible tone will indicate an exposure has been made.

###### Expose

When proper patient positioning is achieved, fully depress the exposure footswitch to the second position. The x-ray tube will begin its prep cycle and upon completion of the prep cycle, the x-ray tube will make an exposure. An audible tone will indicate an exposure has been made. Note that in this procedure an x-ray exposure will not be made immediately upon depressing the footswitch. A delay will be experienced due to the x-ray tube prep cycle.



#### 4.6 Prep/Expose Tubestand Status Messages

- WAIT** Tube is not yet warmed up. Please wait about 2 seconds. Exposures are not allowed yet.
- PREP** The Prep sequence is complete and the system is ready. Exposure starts immediately after initiating with foot switch.
- X-RAY** X-Ray exposure is in progress. Radiation is present.
- DONE** Exposure is completed.
- COLD** Unit needs to warm up for about ten minutes to achieve the most accurate exposure outputs.
- READY** Unit is warmed up and ready for taking exposures.

#### **EXPOSURE COUNT**

With the kVp major, kVp minor and mA selector knobs turned fully counter-clockwise, the bottom display will indicate "EXPO". The KVp display and the mAs display will indicate the total number of exposures taken on this x-ray control.



## 5.0 TECHNICAL DATA

- 5.1 Radiation Leakage (Meets Federal Government Standards)
  - 5.1.1 From the tube housing: less than 50 mR/hr at 1m from focal spot (@4mA, 125kVp)
  - 5.1.2 From collimator: less than 50 mR/hr at 1m (@4mA, 125 kVp)
- 5.2 Rated line voltage: 240 VAC, 60 Hz., single phase.
- 5.3 Range of line voltage regulation at max line current: 1% to 5%.
- 5.4 Maximum line current (based on input voltage of 240 VAC): 140 AMP
- 5.5 Technique factors that constitute the max. line current: 300 mA @ 125 kVp.
  - 5.5.1 Generator rating:
    - 5.5.1.1. Output current: 100-300 mA.
    - 5.5.1.2. Output voltage: 40-125 kVp.
  - 5.5.2 Generator duty cycle:
    - 5.5.2.1. 100 mA @ 125 kVp: 4%
    - 5.5.2.2. 300 mA @ 125 kVp: 1%
- 5.6 Maximum Deviation of technique factors:

The maximum deviation statements provided below are broad and considered "worst case" conditions.

Typical performance will normally be significantly better.



#### 5.6.1 Peak Tube Potential (kVp)

The Maximum Deviation of the Peak Tube Potential during an exposure from its pre-indicated value is + 5 kVp.

#### 5.6.2 Tube Current

The Maximum Deviation of the tube current during an exposure from its pre-indicated value is + 10% of selected value within a kVp range of 50-125 kVp (inclusive), and + 20% of selected value within a kVp range of 40-50 kVp (exclusive).

#### 5.6.3 Exposure Time

The Maximum Deviation of the measured exposure time from its pre-indicated value is  $\pm 1$  pulse for selected times within the range of 1/120-1/10 sec. and  $\pm 15\%$  of selected times within the range of 7/60-2 sec.

### 6.0 **CLEANING THE *INTEGRATED VETERINARY SYSTEM***

The *Integrated Veterinary System* was designed to withstand the sometimes extreme conditions of a busy veterinary practice. In addition to the drip trough and rust-proof table legs, you'll note that there are no grooves or holes to collect debris.

To periodically clean the unit, use a sponge and a non-abrasive cleanser. Knobs on the control panel are removable for this purpose.

The system must be located in a different room than the processor. Failure to observe this could lead to premature corrosion not covered by warranty.



## 7.0 SCHEDULED DEALER MAINTENANCE

The following schedule of maintenance for the *Integrated Veterinary System* is required for safety of operation, continued ease of use, and continued long life of the product.

The maintenance program should only be performed by service personnel authorized by Summit Industries. Frequency of the service should be 30 days after installation and annually thereafter.

### 7.1 X-Ray Generator Maintenance

- 7.1.1 Verify that all technique selector knobs are mounted solidly.
- 7.1.2 Verify proper operation of kVp and mAs digital displays.
- 7.1.3 Verify proper operation of audio and visual x-ray termination.
- 7.1.4 Verify time, mA, and kVp accuracy.
- 7.1.5 Examine all electrical connections of the high voltage generator.
- 7.1.6 Examine oil level of high voltage transformer and refill if fluid level is greater than 3/4" from the top of the lid.
- 7.1.7 Examine the high voltage cable ends for carbon tracking.
- 7.1.8 Examine inside of power supply box for any possible fluid leakage.

### 7.2 X-Ray Tube Housing

- 7.2.1 Inspect for possible oil leakage.
- 7.2.2 Assure that the housing is tightly fastened to the tube mount and collimator.
- 7.2.3 Inspect stator cable for fraying or damage.
- 7.2.4 Inspect high voltage cable ends for carbon tracking. Clean and Regrease HV Cable ends annually.

### 7.3 Collimator

- 7.3.1 Verify accuracy of field size.



- 7.3.2 Verify accuracy of light field to x-ray field alignment.
- 7.3.3 Check lamp on-off switch for proper operation.
- 7.3.4 Inspect collimator cable for fraying or damage.
- 7.4 Tubestand
  - 7.4.1 Verify set-screws are securely holding tubearm.
  - 7.4.2 Inspect counterweight cables for fraying or damage.
  - 7.4.3 Inspect all tubestand movements for binding or interferences.
- 7.5 Other
  - Inspect high voltage cable and all other cabling for damage.



## 8.0 TROUBLESHOOTING

### 8.1 Error Message

Upon error detection, the *Integrated Veterinary System* will display one of the following error codes:

<b>FOOT</b>	Early release of the exposure foot switch during exposure. Films are likely to turn out light. Foot must be depressed for the entire selected exposure time.
<b>TUBE</b>	Single shot tube power limits were exceeded by the selection technique. Reduce kVp, mA and / or time (PREP and EXPOSE locked out). Message clears when the techniques change.
<b>HEAT</b>	Tube heat exceeded. PREP and EXPOSE locked out until technique reduced or tube cools down.
<b>ROTR</b>	Tube rotor error. Call for service.
<b>ZCO</b>	Equipment component (hardware) error. Call for service.
<b>ZZZZ</b>	(Power saver mode only.) Unit will go to sleep within 5 minutes.
<b>FIL1-FIL4</b>	Hardware error. Call for service.
<b>COLD</b>	The unit needs to warm up for best output accuracy, but exposures can be taken if needed. This display should clear about ten minutes after first turn on of the day.

### 8.2 No Exposure

If, after fully depressing the foot switch, there is no audible tone, your unit may not be turned on. Use the circuit breaker to turn on power. If there is still no exposure, call a service representative.

### 8.3 Collimator light bulb burned out.

When the collimator light bulb burns out, you may either call a service person for replacement/realignment or may choose to replace the bulb yourself.

The replacement bulb must be FCS type; 150 Watt at 24 V with a pin base.



**WARNING #1:**

DO NOT LOOK DIRECTLY INTO THE COLLIMATOR LIGHT SOURCE AS RETINA DAMAGE COULD RESULT.

**WARNING #2:**

TURN THE CIRCUIT BREAKER OFF BEFORE ATTEMPTING BULB REPLACEMENT TO AVOID POSSIBLE ELECTRIC SHOCK.

First, remove the back cover of the collimator. The bulb is now visible.

**WARNING #3:**

THE BULB, WHEN LIT, GETS VERY HOT. ALLOW IT TO COOL SEVERAL MINUTES TO AVOID BURNING YOUR FINGERS.

Pull the bulb straight out from the ceramic base.

**WARNING #4:**

DO NOT MAKE DIRECT CONTACT WITH THE REPLACEMENT BULB AS OIL FROM YOUR FINGERS WILL CREATE HOT SPOTS ON THE BULB WHICH SUBSEQUENTLY MAY LEAD TO CRACKING.

To avoid direct contact between bulb and fingers, the replacement bulb is normally packaged in a cellophane wrapper. Tear open one end so that prongs are exposed; hold the glass portion, still in its wrapper, and insert the prongs into the ceramic base. Make sure that each prong is securely fastened into its socket so that the resulting light field is straight. Replace the back cover.

If the light field is out of alignment with the grid cabinet, call an authorized service representative for re-alignment.



8.4 No digital display

If, after turning on the circuit breaker, digital displays do not light up, this indicates lost power. The source may be a blown fuse within the unit or a problem with incoming line power. Call an authorized service representative.

8.5 Circuit tripping

If the circuit breaker shuts off on its own, this indicates mA overload. This could be due to miscalibration of the mA or another malfunction.

In the event that the unit is miscalibrated, you may still be able to operate the unit by moving to 100 mA. This will allow you to take X-Rays until an authorized service representative is called.

8.6 Full kVp range inaccessible.

If this occurs, it means that incoming line voltage is too low. Call an authorized service representative to correct.

8.7 Poor film quality

There are many interrelated factors in the radiographic process which impact the degree of darkening visible on a film. The following is a list of items to check whenever you notice a significant change in film quality:

8.7.1 Film Processing - Has chemistry been changed recently? Is a new brand/type being used? Have developing temperatures varied? All of these affect film quality.

8.7.2 Technique - Were proper technique factors used? Consult with a Summit dealer or call Summit for information on setting up a technique chart.



- 8.7.3 Screens/Cassettes - Screens within the cassettes degrade with time. They typically lose 10% of their light-emitting capability per year. It is recommended that cassettes be re-screened every five to seven years. All screens should be replaced at one time to maintain uniform exposure.
- 8.7.4 Film - Has a new brand/type/speed of film been used? Is the film beyond its expiration date? If so, new film may be purchased or technique factors may need adjustment.
- 8.7.5 Foot switch - If thorax/chest films are blurring more than usual, it could be that the exposure switch is being used incorrectly. See section 4.5 to review how to make exposures.

## 9.0 WARRANTY NOTICE

The *Integrated Veterinary System* is warranted as follows: any Summit manufactured part proving defective will be repaired or replaced free of charge, F.O.B. factory, if the defective part is returned for inspection, freight charges prepaid. This warranty covers parts only and does not include any on-site labor costs.

This warranty is five years from the date of installation.

This warranty does not apply to collimator glassware or x-ray tubes or damage caused by accident, misuse, neglect, or shipment, and is void if service is performed by persons other than authorized Summit dealers or if equipment is interconnected with components not approved by Summit for compatibility.

The x-ray tube manufacturer's warranty is one year, pro-rated. Summit will extend this warranty to five years, pro-rated on manufacturer's list price at time of claim, provided the tube is purchased and used exclusively with an *Integrated Veterinary System*.

**Please call your Summit dealer to coordinate the return of a warranty part or call Summit direct at 1-800-972-9776.**